
This is an electronic reprint of the original article.
This reprint *may differ* from the original in pagination and typographic detail.

Author(s): Tomita, Hideki; Takatsuka, Takaaki; Takamatsu, Takahide; Adachi, Yoshitaka; Furuta, Yujin; Noto, Takuma; Iguchi, Tetsuo; Sonnenschein, Volker; Wendt, Klaus; Ito, Chikara; Maeda, Shigetaka

Title: Development of High Resolution Resonance Ionization Mass Spectrometry for Neutron Dosimetry Technique with $^{93}\text{Nb}(n,n')^{93m}\text{Nb}$ Reaction

Year: 2016

Version:

Please cite the original version:

Tomita, H., Takatsuka, T., Takamatsu, T., Adachi, Y., Furuta, Y., Noto, T., Iguchi, T., Sonnenschein, V., Wendt, K., Ito, C., & Maeda, S. (2016). Development of High Resolution Resonance Ionization Mass Spectrometry for Neutron Dosimetry Technique with $^{93}\text{Nb}(n,n')^{93m}\text{Nb}$ Reaction. In A. Lyoussi (Ed.), ISRD 15 : International Symposium on Reactor Dosimetry. EDP Sciences. EPJ Web of Conferences, 106. <https://doi.org/10.1051/epjconf/201610605002>

All material supplied via JYX is protected by copyright and other intellectual property rights, and duplication or sale of all or part of any of the repository collections is not permitted, except that material may be duplicated by you for your research use or educational purposes in electronic or print form. You must obtain permission for any other use. Electronic or print copies may not be offered, whether for sale or otherwise to anyone who is not an authorised user.

Development of High Resolution Resonance Ionization Mass Spectrometry for Neutron Dosimetry Technique with $^{93}\text{Nb}(n,n')^{93\text{m}}\text{Nb}$ Reaction

Hideki Tomita^{1,2,a}, Takaaki Takatsuka¹, Takahide Takamatsu¹, Yoshitaka Adachi^{1,2}, Yujin Furuta¹, Takuma Noto^{1,2}, Tetsuo Iguchi¹, Volker Sonnenschein³, Klaus Wendt⁴, Chikara Ito⁵, and Shigetaka Maeda⁵

¹ Department of Quantum Engineering, Nagoya University, 464-8603 Nagoya, Japan

² RIKEN Nishina Center, 2-1 Hirosawa, Wako, Saitama 351-0198, Japan

³ Department of Physics, University of Jyväskylä, SF-40351, Finland

⁴ Institute of Physics, Johannes Gutenberg-University Mainz, Staudingerweg 7, 55128 Mainz, Germany

⁵ Oarai Research and Development Center, Japan Atomic Energy Agency, 4002 Narita, Oarai, Ibaraki, 311-1393, Japan

Abstract. We have proposed an advanced technique to measure the $^{93\text{m}}\text{Nb}$ yield precisely by Resonance Ionization Mass Spectrometry, instead of conventional characteristic X-ray spectroscopy. $^{93\text{m}}\text{Nb}$ -selective resonance ionization is achievable by distinguishing the hyperfine splitting of the atomic energy levels between ^{93}Nb and $^{93\text{m}}\text{Nb}$ at high resolution. In advance of $^{93\text{m}}\text{Nb}$ detection, we could successfully demonstrate high resolution resonant ionization spectroscopy of stable ^{93}Nb using an all solid-state, narrow-band and tunable Ti:Sapphire laser system operated at 1 kHz repetition rate.

1. Introduction

Neutron dosimetry in a nuclear reactor is very important to evaluate the irradiation damage of the reactor vessel, structural component and equipment. Conventionally, the neutron activation method has been applied to evaluate neutron dose, which is based on gamma-ray spectrometry of nuclear reaction products. However, nuclear reaction products with short half-lives of less than ten years are not suitable for monitoring the integrated neutron dose over the reactor life time around 40 years or more by the neutron activation method. Alternatively, retrospective nuclear reactor dosimetry has been proposed, which is based on trace analysis of long-lived and stable isotopes produced through nuclear reactions. $^{93}\text{Nb}(n,n')^{93\text{m}}\text{Nb}$ reaction is one of the promising candidates for the dosimetry because it is a threshold reaction desired for measurement of fast neutron fluence and its reaction product $^{93\text{m}}\text{Nb}$ has a suitably long half-life of 16.13 years [1].

^a Corresponding author: tomita@nagoya-u.jp

Resonance ionization mass spectrometry (RIMS), which is based on efficient excitation and ionization via atomic energy levels by tunable laser and subsequent mass spectrometry, is widely applied for trace determination of long-lived radioactive isotopes [2–4]. RIMS for measurement of $^{93\text{m}}\text{Nb}$ yield was proposed so far [5–7] instead of conventional characteristic X-ray spectroscopy. $^{93\text{m}}\text{Nb}$ -selective resonance ionization is achievable by distinguishing the hyperfine splitting of the atomic energy levels between ^{93}Nb and $^{93\text{m}}\text{Nb}$ at high resolution, which depends on $^{93\text{m}}\text{Nb}$ nuclear spin of $1/2^-$ and ^{93}Nb nuclear spin of $9/2^+$ respectively. In this method, cooling time to reduce interference from impurity radioisotopes and complex sample preparation before $^{93\text{m}}\text{Nb}$ measurement would be not necessary. Hyperfine splitting of stable ^{93}Nb was investigated and the expected selectivity on $^{93}\text{Nb}/^{93\text{m}}\text{Nb}$ measurement was already estimated [5–7]. The investigation was based on resonance ionization spectroscopy using conventional dye laser system. To obtain high ion count rate via $^{93\text{m}}\text{Nb}$ -selective resonance ionization, a narrow band-width tunable laser operated at high repetition rate should be used for resonant ionization. However, conventional dye laser system operated at high repetition rate is not suitable for stable long-term operation because degradation of laser dye during operation should be considered carefully.

We developed an all solid-state, narrow-band and tunable Ti:Sapphire laser system, which is based on injection locking [8, 9], operated at repetition rate up to 10 kHz. In addition, some schemes for $^{93\text{m}}\text{Nb}$ selective resonance ionization using this laser system was already found [10]. In advance of $^{93\text{m}}\text{Nb}$ detection, we have investigated high resolution resonance ionization spectroscopy of stable ^{93}Nb using the narrow-band and high repetition rate Ti:Sapphire laser system.

2. Experimental Setup

Figure 1 shows experimental setup for high resolution resonance ionization spectroscopy of stable ^{93}Nb using Ti:Sapphire laser system. Two color – one resonance excitation step scheme, *i.e.* resonance excitation and following non-resonance ionization scheme was used as shown in Figure 2. Second harmonic generation (SHG) of narrow-band Ti:Sapphire laser called injection locked Ti:Sapphire laser and standard Ti:Sapphire laser [11] were used for 1st step resonance excitation (wavelength of 374.345 nm) and non-resonance ionization (wavelength of 357.6 nm) respectively. In this experiment, extended cavity diode laser (ECDL) was used as a master laser of the injection locked Ti:Sapphire laser. The detailed description of the injection locked Ti:Sapphire laser was given in previous papers [5, 6]. The standard Ti:Sapphire laser and the narrow-band Ti:Sapphire laser were pumped by SHG of Nd:YAG laser at repetition rate of 1 kHz. Typical band widths of the standard Ti:Sapphire laser and the narrow-band Ti:Sapphire laser were 3 – 5 GHz and 20 MHz respectively. Inside a vacuum chamber, collimated Nb atom vapor was produced by a hot Nb filament by ohmic heating with a collimator in the diameter of 6.0 mm and introduced into ionization region between two electrodes. Nb atoms were ionized by irradiation of two pulses from the injection locked Ti:Sapphire laser and the standard Ti:Sapphire laser. Nb ions were accelerated by electrostatic fields between electrodes, and then detected by a multi-channel plate (MCP) after 0.6 m field free flight from the ionization region. Ions were counted with time gate of flight time of Nb ion. During ions counting, emission frequency of ECDL, *i.e.* the frequency of the injection locked Ti:Sapphire laser, was measured by a wavelength meter.

3. Results and Discussion

The spectrum of the detected ions was obtained by resonant ionization using the injection locked Ti:Sapphire laser. As a reference, broad spectrum was also obtained using additional standard Ti:Sapphire laser for 1st step instead of the injection locked Ti:Sapphire laser. Figure 3 shows the resonance ionization spectra obtained by frequency scanning of the injection locked Ti:Sapphire laser and the standard Ti:Sapphire laser, respectively. The spectra involved six peaks due to hyperfine

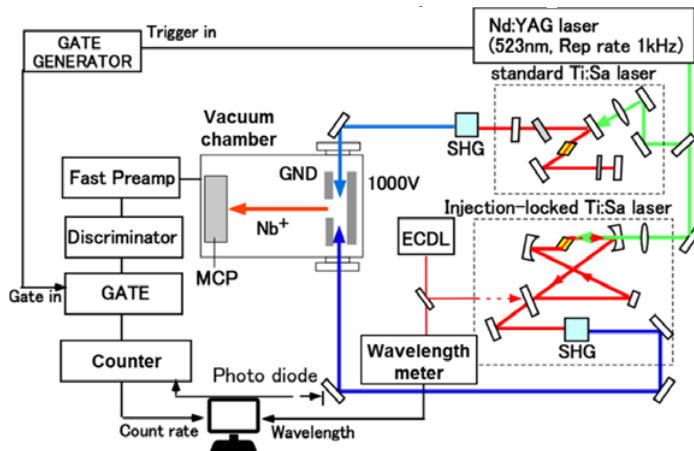


Figure 1. Experimental setup for high resolution resonance ionization spectroscopy of stable ^{93}Nb .

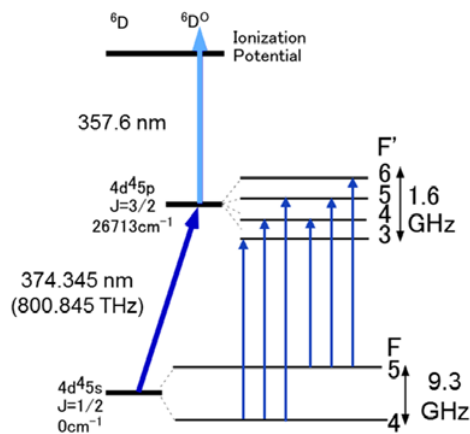


Figure 2. Resonance excitation and ionization scheme of ^{93}Nb .

structures in the lower and upper levels as indicated schematically in Fig. 2. Although the broad spectrum without any hyperfine components was obtained using the standard Ti:Sapphire laser, six peaks were clearly resolved in the spectrum obtained by the injection locked Ti:Sapphire laser. The high resolution spectrum was fit with six Voigt functions as shown in Fig. 3(b). Although Lorentzian component of Voigt fitting due to power broadening in 1st step was not negligible, laser power for 1st step can be reduced in the case of more efficient scheme via additional resonance excitation. Thus, Doppler broadening in atomic vapor was dominant in the line width of the spectrum. In the present setup, average line width of Gaussian component of Voigt fitting was estimated to be 220 MHz. Assuming that additional step via 2nd excited level such as $4d^35s6s\ ^6F_{1/2}$ at 37871.3 cm^{-1} by the injection locked Ti:Sapphire laser was used, selectivity in $^{93\text{m}}\text{Nb}$ resonance ionization of 10^5 would be achievable. Uncertainty of a few percent would be possible if some correction for laser frequency is applied [12]. In addition, systematic error would be reduced because the ratio of $^{93\text{m}}\text{Nb}/^{93}\text{Nb}$ is directly measured by RIMS.

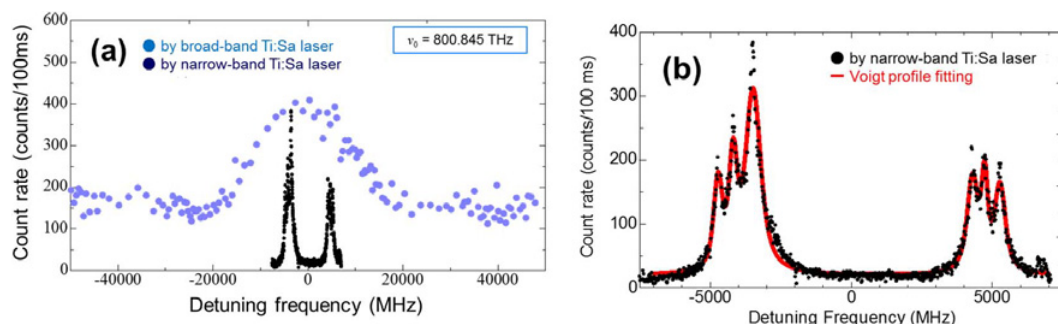


Figure 3. (a) Resonance ionization spectra obtained by frequency scanning of the injection locked Ti:Sapphire laser and the standard Ti:Sapphire laser respectively, (b) high resolution spectrum with six Voigt profile fitting. The center frequency of the injection locked Ti:Sapphire laser was 800.845 THz (374.345 nm).

4. Conclusions and Future Work

High resolution resonance ionization spectroscopy method by high repetition rate Ti:Sapphire laser system was developed toward precise $^{93\text{m}}\text{Nb}$ yield measurement. We successfully demonstrated high resolution resonance ionization spectroscopy of stable Nb using the present laser system, in which hyperfine splitting was resolved clearly. Such high resolution spectroscopy is required for optical separation of $^{93\text{m}}\text{Nb}$ signal from stable ^{93}Nb signal and expected selectivity would be 10^5 . Uncertainty in isotope ratio measurement by RIMS would be expected less than a few percent with proper correction method applied. Isotope analysis by high resolution RIMS might possibly be applied to the transmutation detectors used for neutron fluence measurement [13, 14].

High resolution spectroscopy using additional narrow-band Ti:Sapphire laser will be performed to demonstrate the optical selectivity of 10^5 . We are now developing a supersonic gas-jet atomic source to make uniform velocity of sample atoms for higher efficiency resulting from better spatial overlap with laser irradiation and also for higher selectivity resulting suppression of Doppler broadening in the spectroscopy [15]. Gas-jet atomic source will also be involved. In addition, overall efficiency of the measurement will be verified experimentally with Nb dosimeters of the fast experimental reactor JOYO at Japan Atomic Energy Agency, Japan.

This work was supported by JSPS KAKENHI Grant Number 26420868.

References

- [1] L. Greenwood, *et al.*, J. Nucl. Mater, **361**, 1–9 (2007)
- [2] V. S. Lethokov, *Laser Photoionization Spectroscopy*, Academic Press, Orlando (1987)
- [3] G. S. Hurst and M. G. Payne, *Principles and Application of Resonance Ionisation Spectroscopy*, Adam Hilger, Bristol (1988)
- [4] Radioisotope Mass Spectrometry in *Handbook of Radioactivity Analysis*, Edit. M. Annunziata, Academic Press, Amsterdam, 799–845 (2003)
- [5] H.M. Lauranto, *et al.*, Applied Physics B **50**, 323–329 (1990)
- [6] H.M. Lauranto, *et al.*, Spectrochimica Acta Part B **51**, 175–180 (1996)
- [7] H.M. Lauranto, Appl. Phys. B **66**, 231–239 (1998)
- [8] H. Tomita, *et al.*, J. Nucl. Sci. Tech. **suppliment6**, 37–42 (2008)
- [9] T. Kessler, *et al.*, Laser Physics **18**, 842–849 (2008)

- [10] T. Takatsuka, *et al.*, Hyperfine Interactions **216**, 41–46 (2013)
- [11] S. Rothe *et al.*, Journal of Physics: Conference Series **312**, 052020 (2011)
- [12] T. Noto and H. Tomita *et al.*, *to be submitted*
- [13] L. Viererbl *et al.*, Nucl. Instrum. Meth. A **632**, 109–111 (2011)
- [14] V. Klupák *et al.*, “Nickel foil as transmutation detector for neutron fluence measurements”, in ISRD15 proceedings, E153 (2014)
- [15] T. Takatsuka, *et al.*, Nucl. Instrum. Meth. B **317**, 586–589 (2013)